

SRP-300

Digital Bench Scale

Operation Manual

Revision 1.2
August 24, 2000

Transcell Technology inc.

© 1995-2000 Transcell Technology, Inc.

Contents subject to change without notice.

Transcell Technology, Inc.
975 Deerfield Parkway
Buffalo Grove, IL 60090
Tel (847) 419-9180
Fax (847) 419-1515
E-mail: transcell@transcell.net
Web: www.transcell.net

Table of Contents

Introduction	1
Installation and Wiring	1
Keyboard Functions	2
Configuration.....	2
User Menu Descriptions	3
Calibration	4
Displayed Error Messages	4
Specifications	5
Warranty and Service Information.....	6

Introduction

The SRP Series Digital Bench Scale is a large (18" x 18") bench scale with remote digital indicator. The system is NTEP-certified for Class III at 3,000 divisions, and is legal-for-trade. Housed in a standard black polymer case, the indicator displays its numerals on a bright VFD screen. The base unit features a removable stainless steel platform, an RS-232 serial communication port, and adjustable feet for leveling.

The SRP Series uses full duplex RS-232 serial format for communication with many types of attached support equipment. The

unit can transmit data on demand, or continuously in several popular data protocols to match a wide variety of printers, remote displays, or personal computers. If you plan to use your scale with equipment other than a PC, you may have to alter the serial communication parameters that are embedded in the User Menu.

The User Menu is accessed through the front panel keys. Complete directions, including a graphical road map, are found in the Configuration section of the manual.

Installation and Wiring

Unless you wish to interface to a device other than a PC, no wiring is necessary. Simply connect the indicator to the scale platform, plug in the AC adapter, and turn the unit on. If the swivel indicator option was ordered, the stainless steel post may be mounted to the bottom of the base with the hardware provided. Alternately, it may be mounted to a table or bench. In general,


please allow a 20-minute warm up period before using the scale.

If interfacing to a PC, simply connect the optional null modem cable to a serial port (e.g. COM 1) on your PC. If your computer has a 25-pin serial port, a standard 9-pin to 25-pin adapter, such as the type used for a mouse, may be used and is readily available at your local computer supply retailer.

If interfacing to a serial device other than a PC, you may have to wire your own cable to communicate with that device. If so, refer to the 9-pin connector pin out shown at right.

Pin No.	Pin Name
2	Receive Data
3	Transmit Data
5	Signal Ground

Keyboard Functions



Toggles between lb and kg units if this key is enabled in the User Menu.



Sets indicator to display "0" when in Gross mode, and within zero band range.




Toggles between Gross and Net weight display.



Used to zero a weight indication in Net mode.



Sends "Print" data to printer if scale is stable and not in overload. Not active when "Continuous" option is selected in User Menu.

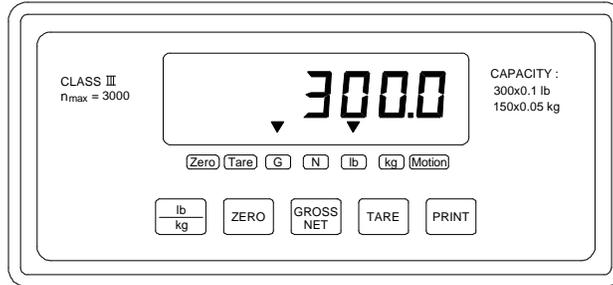

SRP SERIES FRONT PANEL


Configuration

All Serial Communication parameters are embedded in a user menu consisting of 5 separate menu selections, each with its own sub-menu of choices. If your scale is connected by RS-232 serial communication lines to other equipment, or you wish to disable the **lb/kg** key, you may have to modify some or all of these parameters.

To modify these parameters, you must first enter the USER MENU mode. Once there, four of the front panel keys become directional navigators to move around in the menus, and one key is used to save or SET the selections. Complete directions are found below.


To place the unit in USER MENU mode:

1. Turn the scale off.
2. While holding down the **lb/kg** key, turn the scale back on.
3. When the display shows "A1", the unit is in USER MENU mode, and you can release the **lb/kg** key. Shown at right are the directional and SET key assignments.

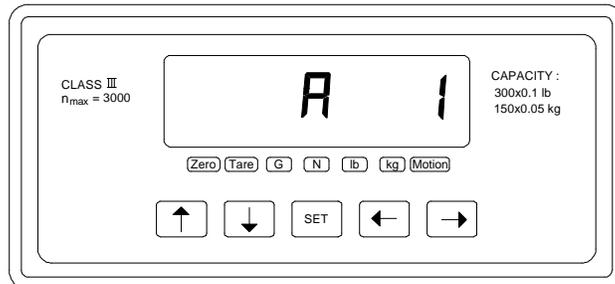

Configuration / Continued

USER MENU CHART

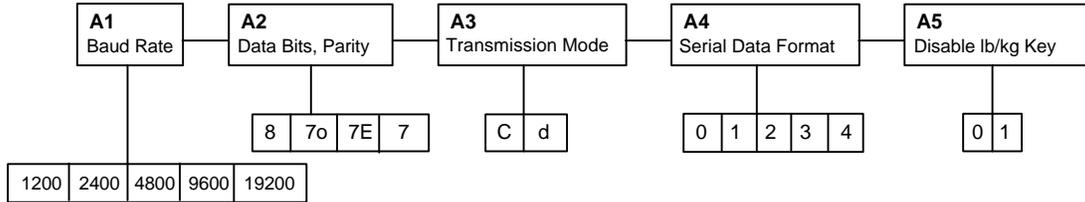

To place the unit back into the **NORMAL OPERATING** mode, turn off the power to the unit. With no keys held down, turn the power back on. All front panel keys will now return to their normal mode of operation.

User Menu Descriptions

NAME/CODE	DESCRIPTION	CODE/VALUE
A1 Baud Rate	Selects the baud rate for data transmission through the serial port.	1200 2400 √ 4800 9600 19200
A2 Data Bits and Parity	Selects the number of data bits and parity of serial transmission. "8" = 8 data bits with no parity bit and one stop bit "7O" = 7 data bits with odd parity bit and one stop bit "7E" = 7 data bits with even parity bit and one stop bit "7" = 7 data bits with no parity bit and two stop bits	8 √ 7O 7E 7
A3 Mode of Serial Transmission	Selects when data will be sent out of the serial port to a printer or computer: "C" = Continuous mode; send data continuously "d" = Demand mode; send data when a PRINT command is issued from the printer, computer, or indicator.	C √ d
A4 Serial Data Format	Selects the data format to be transmitted via the serial port to a printer or computer. "0" = Consolidated Controls Format "1" = Toledo 8213 Format "2" = NCI 3825Format "3" = Transcell Technology Format "4" = Fairbanks 70-2453-4 Format	0 1 2 3 √ 4
A5 Disable the lb/kg Key	Allows the lb/kg key to be disabled so that an operator cannot accidentally press the key and change the displayed units. "0" = Disable the lb/kg key "1" = Enable the lb/kg key	0 1 √

Calibration

All SRP Series scales may be calibrated with any precision test weight from 10% to 100% of the scale's capacity. The recommended test weight is about 2/3 of the full-scale capacity, but in general, the larger the test weight, the more accurate the scale will be. The only restriction is that the test weight *must* be in pounds.

1. Turn the scale off. Locate the hidden switch on the base panel and set it at the rightmost position. Turn the unit back on. The message "C 0" appears on the display briefly, followed by a value which remains on the screen. Allow a 20 minute warm-up period for the load cell and indicator to become thermally stable.
2. Press **ZERO** to zero the value, then press the **NET/GROSS** key to save the zero point value.
3. The display will momentarily prompt "C 1" for the span calibration, followed by "0. 0" with one digit flashing. Place the test weight on the platform.
4. Use the four directional keys to adjust the displayed value to the actual test weight value in pounds. Increase the flashing digit by pressing the **lb/kg** key. Decrease the flashing digit by pressing the **ZERO** key. Pressing the PRINT key or the TARE key can change the position of the flashing digit.
5. After setting the exact value, press the **NET/GROSS** key to save the value.
6. If the calibration was successful, the display will show "ECAL" momentarily, then freeze. Exit the Calibration mode and enter the Normal Operating Mode by turning off the scale, positioning the calibration switch back to the leftmost position, and turning the scale back on.
7. If the calibration was *not* successful, one of the error messages below will appear. Take the indicated action to correct the problem, then perform a new calibration.

"Err0" - The calibration test weight or the adjusted keyed-in weight is larger than full scale. Change the calibration test weight or check the keyed-in weight.

"Err1" - The calibration test weight or the adjusted keyed-in weight is smaller than 10% of full scale. Change the calibration test weight or check the keyed-in weight.

"Err2" - Check keyed-in weight with the actual weight placed on platform.

Displayed Error Messages

Display Message	Cause or Condition
-HI-	Scale was turned on with a weight on the platform that exceeded the Zero Capture Range. Scale must be turned on without extra weight on the platform.
-LO-	Scale was turned on without stainless steel platform on scale base that exceeded the Zero Capture Range in the negative direction. Replace platform and restart.
□□□□□	Total weight on platform exceeds scale's capacity.
-----	During normal operation, the stainless steel platform was removed, resulting in an under range condition. Replace scale platform.

Specifications

CONSTRUCTION:

Indicator: Black ABS with steel back plate.

Base: Steel with stainless steel platform.

DISPLAY:

7 Digit, 0.5", 7-Segment
Vacuum Fluorescent

NIST CLASSIFICATION:

Meets H-44 Class III at 3,000 divisions

OVER CAPACITY ANNUNCIATION:

103% of Full Scale Capacity

OPERATING TEMPERATURE RANGE:

14°F to 104°F
(-10°C to 40°C)

OPTIONAL SWIVEL POST:

18" Tall
Stainless Steel Construction

POWER SOURCE:

AC Adapter, 12VDC, 800mA,
included


WEIGHT:

Net Weight: 45 lb (20.4 kg)
Shipping Weight: 50 lb (22.7 kg)




Certificate of Conformance
#95-034

PHYSICAL DIMENSIONS:

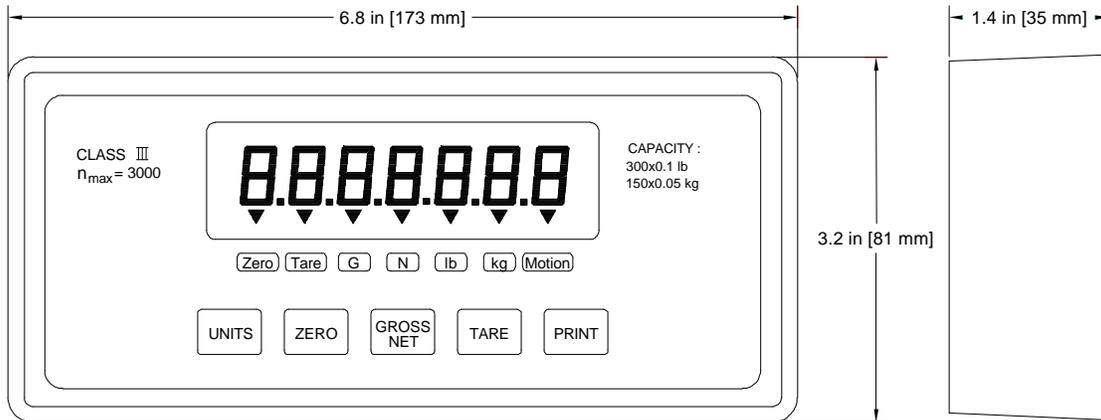

REMOTE INDICATOR

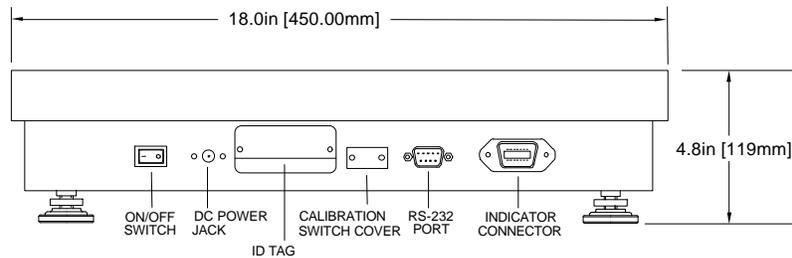

BASE

Warranty and Service Information

Seller warrants that the SRP Series Digital Electronic Bench Scale will conform to written specifications, drawings, and other descriptions made by the manufacturer, including any modifications thereof. The Seller warrants the goods against faulty workmanship and defective materials. If any goods fail to conform to these warranties, Seller will, as its sole and exclusive liability hereunder, repair or replace such goods if they are returned within the following warranty period:

Twelve (12) months from date of shipment from manufacturer.

These warranties are made upon the express condition that:

- 1) Transcell Technology, Inc. is given prompt written notice upon discovery by Buyer of such non-conformity, with a detailed explanation of the alleged deficiencies;
- 2) Such goods are returned to the Seller at the expense of the Buyer;
- 3) Examination of such goods by Seller discloses that the nonconformity actually exists and was not caused by accident, misuse, neglect, alteration, improper installation improper or unauthorized repair, or improper testing, and
- 4) Such goods have not been modified, altered, or changed by any person other than the Seller or its duly authorized repair agents.
- 5) Transcell Technology, Inc. will have a reasonable time to repair or replace such goods.

THESE WARRANTIES EXCLUDE ALL OTHER WARRANTIES, EXPRESS OR IMPLIED, ORAL OR WRITTEN, INCLUDING WITHOUT LIMITATION WARRANTIES OF MERCHANTABILITY OR FITNESS FOR A PARTICULAR PURPOSE. SELLER WILL NOT IN ANY EVENT BE LIABLE FOR INCIDENTAL OR CONSEQUENTIAL DAMAGES.

IN ACCEPTING THIS WARRANTY, THE PURCHASER OR BUYER AGREES TO WAIVE ANY AND ALL OTHER CLAIMS FOR RIGHT TO WARRANTY FROM TRANSCCELL TECHNOLOGY, INC. SHOULD THE SELLER BE OTHER THAN TRANSCCELL TECHNOLOGY, INC., THE BUYER AGREES TO LOOK ONLY TO THE SELLER FOR WARRANTY CLAIM OR CLAIMS.

No terms, conditions, understanding, or agreements purporting to modify the terms of this warranty shall have any legal effect unless made in writing and signed by a corporate officer of the Seller.